

欢乐童年....
健康成长



海豹
Seal



七星瓢虫
Ladybug



口腔灯
operating light



刺猬
Hedgehog



长颈鹿
Giraffe



孔雀
Peacock



蝎子
Scorpion



海星
Starfish



羚羊
Antelope

出厂配置

★24V静音直流电机	一套
★冲痰漱口定量给水自动系统	一套
★ 豪华新型材料痰盂（防摔/可拆卸）	一套
★ 8孔豪华LED口腔灯(白光/黄光)	一盏
★ 三用喷枪（冷/热）	二支
★ 电动牙科椅控制系统（9个记忆）	一套
★ 水气电总开关装置地箱	一套
★移动式工具盘	一套
★进口电磁阀	一套
★ LED观片灯	一套
★医生转椅 C型	一张
★铸铝多功能脚踏开关	一套

STANDARD ACCESSORIES

★24V noiseless DC motor	1set
★Auto spittoon flush and cup filler control system	1set
★ Luxury spittoon(detachable)	1set
★ 8 holesLuxury LED light(White light/yellow light)	1set
★3-way syringe(Cold/hot water)	2set
★ Luxury motor chair control system with nine memory	1set
★ Floor box with main switch(Air/Water)	1set
★ Removable instrument tray	1set
★ Imported electromagnetism valve	1set
★ LED x-ray film viewer	1set
★ Dentist stool C	1set
★Cast aluminum multi-function foot switch	1set

技术参数

★ 电源电压	220V-50HZ/60HZ
★ 电机电压	24V
★ 气源气压	0.5MPa-0.8MPa
★ 水源水压	0.2MPa-0.4MPa

SPECIFICATIONS

★ Power Voltage	220V-50HZ/60HZ
★ Motor Voltage	24V
★ Air Pressure	0.5MPa-0.8MPa
★ Water Pressure	0.2MPa-0.4MPa



欢乐童年....
健康成长



裕键板
Keyboard



口腔灯
operating light



靠背安全锁
Backrest safety lock



束缚带
restraint belt



痰盂
Spitton




多功能脚踏
Multifunctional foot control



急停开关
Emergency stop switch



转换开关
Transfer switch



可伸缩脚垫
retractable feet

出厂配置

★24V静音直流电机	一套
★冲痰漱口定量给水自动系统	一套
★ 豪华新型材料痰盂（防摔/可拆卸）	一套
★ 豪华LED口腔灯(白光/黄光)	一盏
★ 三用喷枪（冷/热）	二支
★ 电动牙科椅控制系统（3个记忆）	一套
★ 水气电总开关装置地箱	一套
★移动式工具盘	一套
★进口电磁阀	一套
★ LED观片灯	一套
★医生转椅 C型	一张
★铸铝多功能脚踏开关	一套

STANDARD ACCESSORIES

★24V noiseless DC motor	1set
★Auto spittoon flush and cup filler control system	1set
★ Luxury spittoon(detachable)	1set
★ Luxury LED light(White light/yellow light)	1set
★3-way syringe(Cold/hot water)	2set
★ Luxury motor chair control system with three memory	1set
★ Floor box with main switch(Air/Water)	1set
★ Removable instrument tray	1set
★ Imported electromagnetism valve	1set
★ LED x-ray film viewer	1set
★ Dentist stool C	1set
★Cast aluminum multi-function foot switch	1set

技术参数

★ 电源电压	220V-50HZ/60HZ
★ 电机电压	24V
★ 气源气压	0.5MPa-0.8MPa
★ 水源水压	0.2MPa-0.4MPa

SPECIFICATIONS

★ Power Voltage	220V-50HZ/60HZ
★ Motor Voltage	24V
★ Air Pressure	0.5MPa-0.8MPa
★ Water Pressure	0.2MPa-0.4MPa

儿童椅 – 实例图 Instance Diagram















儿童椅 – 实例图 Instance Diagram

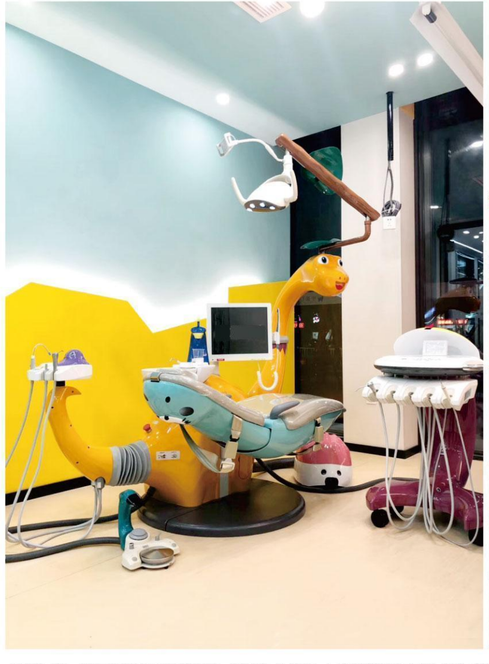








版面有限，以下所列并非所有用户，排名不分先后，最终解释权归安业医疗 器械有限公司所有。

儿童牙椅结构施工图


SHOP DRAWING FOR REFERENCE

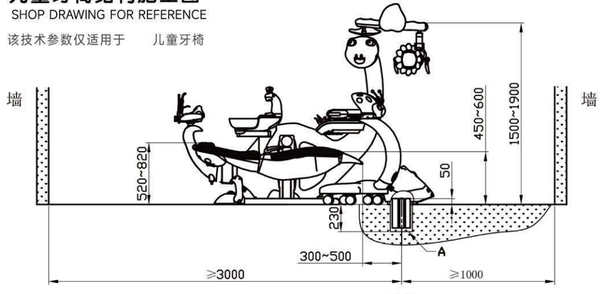该技术参数仅适用于　儿童牙椅



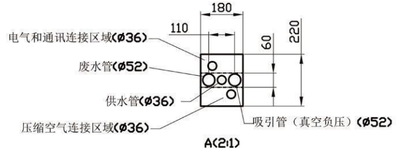

A(2:1)

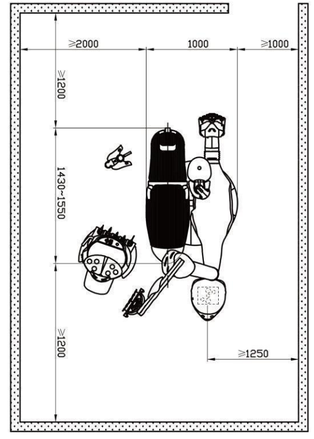

保养与维护

★使用的水要要干净清洁，以免造成牙椅内部管路及阀门堵塞。

★空压机要经常排水，时间久了不排水会造成空压机排出的气中有大量的水分，导致牙椅气路老化或堵塞。(一月排一次为宜)

★电机长期工作后要润滑保养，可用黄油涂抹伸缩处。（半年一次为宜）

★尽量避免病人身上的锋利物品划破椅面。

★不要在电源不稳定的情况下使用牙椅，以免损坏牙椅内部电子部件。

★夏天天气炎热时可拔开热水器开关；冬天零下低温时，应排出热水器里剩下的储水，避免冻裂热水器。

★每天工作完后切记一定要关闭电源和水气开关。

MAINT ENANCE

★In order to avoid blocking of the internal tubing and valve for dental unit, you should use the clear water.

★You should pay attention to draining sewage. there is moisture in the air, according to the local air humidity ,you should drain dirty water once about one month (when large loadwork ,should be half month).

★ Dental chair is still the integration stage between machine and motor ,so you should lubricate the motor when use it about half year.

★Trying your best to avoid lacerating the cushion by the key or other edge tool of patient .

★Do not use the dental chair in the event of power supply instability, so as not to damage the electronic parts inside of the dental chair.

★In summer,could unplug the water heater in the box (could consult the local distributor); when it is low temperature below zero in winter ,while it is out of work ,please blow inside water to be dry ,otherwise the water heater may freeze to damage under the very low temperature during the nigh.

★For the dental unit ,after a day of work , must be cut off electricity,broken water,broken gas and sanitized.